

21.04.2025

Service Order Report: 45189034

Customer / Hospital	Job Information
คณะทันตแพทยศาสตร์ จุฬาลงกรณ์มหาวิทยาลัย จังหวัดกรุงเทพมหานคร 10330	Order Type: Service Repair - On-Site Product line: IC Healthcare Engineer Responsible: Patiphan Chayket Informed by:

Equipment Information	
Description: STEAM STERILIZER GSS67H Material Code / Model: 67H172E Equipment Serial No: 0011219348-010-02	Customer ID / Machine ID: Location: Room:

Fault / Customer Requirement
Sterilizer ระบบดูดอากาศผิดปกติ

Inspection / Correction Actions / Remarks / Recommendations
ลูกค้าย้ำแจ้งอาการvacuum timeout ตรวจเช็คกราฟพบว่าค้างอยู่ที่ 0.5bar ตรวจเช็คชุดอุปกรณ์ positioner เริ่มทำงานผิดปกติ ทำการแก้ไขเบื้องต้นแล้วทดสอบใหม่อีกครั้ง ยังมีอาการเพิ่มเติมคือยังคง vacuum ค้างที่ 0.1bar ตรวจเช็คเพิ่มเติมพบว่าชุดปั๊มแวกคัมเริ่มเสื่อมสภาพ ทำการแก้ไขให้เครื่องสามารถใช้งานได้ Tool Service TRUE RMS CLAMP METER FLUKE 323 S/N: 39690602WS Date Cal. 24-jul-2024 Date Due. 24-jul-2025 Certificate No: EL-24-0207


Declared / Replaced Part Details			
Component	Part No.	Quantity	Remarks

Consumed Time

21.04.2025

Service Order Report: 45189034

Date	Time in	Time out	Hours	Engineer Name	Remarks
18.04.2025	13:00	17:00	4	Patiphan Chayket	BILLABLE
18.04.2025	17:30	20:00	2.5	Patiphan Chayket	BILLABLE

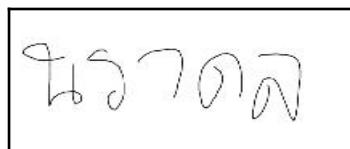


นรทล

Customer's signature

Email:

chomnuch78@gmail.com

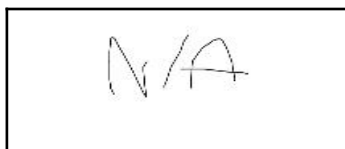

N/A

BIOMED Engineer

Email:



patiphan

Getinge Representative

Email:

patiphan.chayket@getinge.com